

BioSim™ Rituximab (Human) ELISA Kit

rev 12/20

(Catalog # E4371-100, 96 assays, Store at 4°C)

I. Introduction:

Rituximab (Mabthera®) is a genetically engineered chimeric murine/human monoclonal antibody specific to CD20. CD20 is an approximately 35 KDa transmembrane phosphoprotein involved in the activation, proliferation, and differentiation of B-lymphocytes. It is absent in terminally differentiated plasma cells. The Fab domain of rituximab binds to the CD20 antigen on B-lymphocytes and the Fc domain recruits immune effector functions to induce apoptosis in B cells and is used in the treatment of leukemia s and lymphomas, some autoimmune disorders, and organ transplant. BioVision's BioSim™ Rituximab ELISA kit is designed to quantify/measure the Rituximab with high specificity and sensitivity in biological matrices.

II. Application:

This ELISA kit is used for *in vitro* quantitative determination of Rituximab.

Detection Range: 3 - 300 ng/ml

Sensitivity: 3 ng/ml

Assay Precision: Intra-Assay: CV < 30%; Inter-Assay: CV < 30% (CV (%) = SD/mean X 100)

Cross Reactivity: No significant cross-reactivity or interference with other proteins present in native human serum or other therapeutic immunoglobulins.

Recovery rate: < 100 ± 30% with normal human serum samples with known concentrations

III. Sample Type:

Human serum and plasma

IV. Kit Contents:

Components	E4371-100	Part No.
Micro ELISA Plate	1 plate	E4371-100-1
Rituximab Standards (S1 – S8)	1 ml X 8	E4371-100-2.x
Assay Buffer	2 x 50 ml	E4371-100-3
HRP-conjugate Probe	12 ml	E4371-100-4
TMB substrate (Avoid light)	12 ml	E4371-100-5
Stop Solution	12 ml	E4371-100-6
Wash buffer (20X)	50 ml	E4371-100-7
Plate sealers	2	E4371-100-8

V. User Supplied Reagents and Equipment:

- Microplate reader capable of measuring absorbance at 450 nm
- Calibrated measures
- Precision pipettes with disposable tips
- Clean eppendorf tubes for preparing standards or sample dilutions
- Absorbent paper

VI. Storage and Handling:

The entire kit may be stored at 4°C for up to 12 months from the date of shipment.

VII. Reagent and Sample Preparation:

Note: Prepare reagents within 30 minutes before the experiment.

Before using the kit, spin tubes and bring down all components to the bottom of tubes.

1. **Wash Buffer:** Dilute the 20X Wash Buffer to 1X solution in ddH₂O (10 ml of Wash Buffer stock to 190 ml of ddH₂O). Mix the 1X solution thoroughly by vortex manually. The working stock can be stable for 2 weeks after preparation at 4°C.

2. **Standard Preparation:**

Ready to use

Name	S1	S2	S3	S4	S5	S6	S7	S8
Conc. (ng/ml)	300	100	30	10	3	0	High Standard	Low Standard

3. **Sample Dilution:**

- **Serum/Plasma:** First dilute samples at 1:10 (10 µl Serum/Plasma + 90 µl Assay Buffer). Secondly, dilute samples 1:100 (5 µl diluted sample + 495 µl Assay Buffer) (Dilution factor : 1000)
- Diluted samples should further be diluted if the concentration of rituximab is higher than the measuring range.
- The usual precautions for venipuncture should be observed. Samples are stable at 4°C for 7 days and -20°C for 6 months. Avoid freeze-and-thaw cycle.

FOR RESEARCH USE ONLY! Not to be used on humans.

VIII. Assay Protocol:

Note: Bring all reagents, microplate and samples to room temperature 15 minutes prior to the assay.

It is recommended that all standards and samples be run at least in duplicate.

A standard curve must be run with each assay.

1. Prepare all reagents, samples and standards as instructed in section VII.
2. Add 100 μ l of **standards** and **diluted-samples** into appropriate wells. Cover wells and incubate for 60 minutes at room temperature (RT).
3. Discard incubation solution. Wash plate 3 times each with 300 μ l of diluted **Wash Buffer**. Remove excess solution by tapping the inverted plate on a paper towel.
4. Add 100 μ l of **HRP-conjugate** into each well. Cover wells with adhesive plate sealer and incubate at RT for 60 minutes.
5. Discard the solution and wash the wells as step 3.
6. Add 100 μ l of 1X **TMB substrate** solution and incubate the plate in dark at RT for 15 minutes
7. Add 100 μ l of **Stop solution** to stop the reaction
8. Read the absorbance in micro plate reader set to 450 nm within 20 minutes. (reference wavelength to 650 nm)

IX. CALCULATION:

Using the standards (300; 100; 30; 10; 3; 0 ng/mL) disregarding zero standard, construct a standard curve by plotting the OD_{450/650} nm for each of 5 standards on the Y-axis versus the corresponding rituximab concentration on the X-axis. Construct a standard curve of difference data using software capable of generating four parameter logistic (4PL) or point-to-point calculation curve fit. To obtain the exact values of the samples, the concentration determined from the standard-curve should be multiplied by the dilution factor.

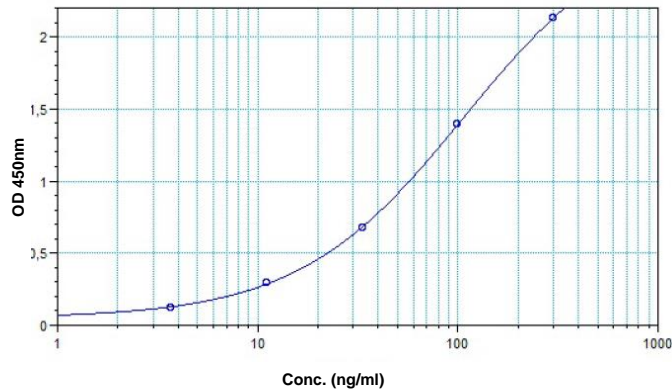


Figure: Typical Standard Curve: These standard curves are for demonstration only. A standard curve must be run with each assay.

X. RELATED PRODUCTS:

- BioSim™ Rituximab (Human) ELISA Kit (Cat. No. E4371-100)
- BioSim™ Adalimumab (Human) ELISA Kit (Cat. No. E4372-100)
- BioSim™ Bevacizumab (Human) ELISA Kit (Cat. No. E4373-100)
- BioSim™ Etanercept (Human) ELISA Kit (Cat. No. E4374-100)
- BioSim™ anti-HER2 (Human) ELISA Kit (Cat. No. E4376-100)
- BioSim™ Golimumab (Human) ELISA Kit (Cat. No. E4377-100)
- BioSim™ Cetuximab (Human) ELISA Kit (Cat. No. E4379-100)
- BioSim™ Denosumab (Human) ELISA Kit (Cat. No. E4380-100)
- BioSim™ Omalizumab (Human) ELISA Kit (Cat. No. E4381-100)
- BioSim™ Nivolumab (Human) ELISA Kit (Cat. No. E4382-100)
- BioSim™ Pembrolizumab (Human) ELISA Kit (Cat. No. E4383-100)
- BioSim™ Ipilimumab (Human) ELISA Kit (Cat. No. E4384-100)

FOR RESEARCH USE ONLY! Not to be used on humans.